

**GenieFluor 647 Anti-Human CD235  
Antibody [HIR2]**  
Catalogue Code: AGEL1098

**Antibody Data**

<b>Product SKU:</b>	<b>AGEL1098</b>	<b>Clone:</b>	<b>HIR2</b>
<b>Applications:</b>	<b>FCM</b>		
<b>Reactivity:</b>	<b>Human</b>		

**Important Note:**

Centrifuge before opening to ensure complete recovery of vial contents.

**Product Information:**

**Alternate Names:** Glycophorin-A/B;GYPA/B;MN sialoglycoprotein;SS-active sialoglycoprotein;PAS-2/3;Sialoglycoprotein alpha/delta;CD235a/b;

**Uniprot ID:** P02724 P06028

**Background:** The HIR2 antibody reacts with a common epitope of glycophorin A (CD235a) and glycophorin B (CD235b). Glycophorin A is the major sialoglycoprotein expressed on red blood cell membrane, and erythroid precursors. Glycophorin A shares strong homology with glycophorin B. The HIR2 antibody recognizes human RBCs and erythroid precursors and is useful in erythroid cell development studies. Mature, non-nucleated red blood cells are characteristically glycophorin A positive, but CD45 and CD71 negative.

**Form:** Liquid


**Conjugation:** Genie Fluor647

**Size:** 20 Tests, 100 Tests, 200 Tests

**Host Species:** Mouse

**Isotype:** Mouse IgG2b, κ

647 Excitation and Emission Spectra

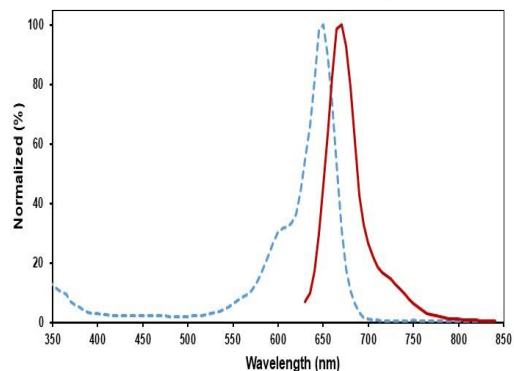

**Isotype Control:** Genie Fluor 647 Mouse IgG2b, κ Isotype Control[MPC-11] [Product AGEL1098]

**Storage Buffer:** Phosphate buffered solution, pH 7.2, containing 0.09% stabilizer and 1% protein protectant.

**Shipping:** Biological ice pack at 4°C

**Stability & Storage:** Keep as concentrated solution. Store at 2~8°C and protected from prolonged exposure to light. Do not freeze. Centrifuge before opening to ensure complete recovery of vial contents. This product is guaranteed up to one year from purchase.

**Recommended Usage:** Each lot of this antibody is quality control tested by flow cytometric analysis. The amount of the reagent is suggested to be used 5  $\mu$ L of antibody per test (million cells in 100  $\mu$ L staining volume or per 100  $\mu$ L of whole blood). Please check your vial before the experiment. Since applications vary, the appropriate dilutions must be determined for individual use.